

Premolars restored with posts of different materials: fatigue analysis

Pablo-Jesús RODRÍGUEZ-CERVANTES¹, Joaquín-Luis SANCHO-BRU¹, Carmen GONZÁLEZ-LLUCH¹, Antonio PÉREZ- GONZÁLEZ¹, Amaya BARJAU-ESCRIBANO² and Leopoldo FORNER-NAVARRO²

¹Department of Mechanical Engineering and Construction, University Jaume I, E-12071, Castellón de la Plana, Spain

²Department of Stomatology, University of Valencia, E- 46010, Valencia, Spain

Corresponding author, Pablo-Jesús RODRÍGUEZ-CERVANTES; E-mail: cervante@emc.uji.es

Previous works studied the effect of the material and the dimensions of the post on the biomechanical performance (fracture strength and stress distribution) of restored teeth, under static loads. The aim of this work was to study the effect of the post material (glass fibre and stainless steel) on restored teeth, which have the final crown, under dynamic conditions. The use of a biomechanical model, including a fatigue analysis from FEA, is presented as a powerful method to study the effect of the material of the intraradicular post. The inclusion of the fatigue analysis allows for a more realistic study that takes into account the dynamic nature of masticatory forces. At the same time, the results obtained are easier to interpret by both dentists and mechanical engineers. No differences were found, with the load and number of cycles considered, between glass fibre and stainless steel as material for the intraradicular post used in premolars restorations.

Keywords: Fatigue, Restored teeth, Prefabricated intraradicular posts, Influence of post material, FEA

INTRODUCTION

Endodontically treated teeth have less moisture in the calcified tissue than vital teeth, which leads to increased brittleness¹. The ability of a post and core system to survive masticatory forces (the instantaneous loading over time) and remain firmly seated in the tooth is critical to the survival of a restoration. If either the post and/or the core material fails, the crown will ultimately fail. Therefore, the retention of a post and the stability of a core is an important factor in preventing restoration failures. Much of the literature has described techniques and methods for the construction of posts and cores including cast systems and prefabricated post systems^{2,3}.

Traditionally, a porcelain fused-to-metal crown has been used in tooth restoration, when an aesthetic appearance is required. However, because of concerns about allergic reactions or biocompatibility⁴, patients and dentists have come to prefer metal-free restorations. It is possible to replicate the aesthetic characteristics and vitality of natural teeth by using ceramics⁵. The major problem with all-ceramic full crowns is to provide excellent aesthetics and adequate strength, *i.e.*, longevity at the same time. Ceramic materials are superior in terms of permeability to light and biocompatibility, but they can be inherently brittle and weak when placed under tensile and torsional stresses⁶. This drawback has been reduced using reinforced glass-ceramic materials. Survival rates of glass-ceramic crowns, even on posterior teeth, have far exceeded those of traditional all-porcelain crowns, despite having nearly equivalent strengths and thicknesses⁷.

Although clinical trials would be the best way to assess the effects of different variables, this type of study

is time consuming, expensive and ethically questionable. Other types of study are helpful, including *in vitro* studies and finite element analyses (FEA). Both methods have advantages and disadvantages. *In vitro* tests can simulate almost realistic conditions, but are time consuming and only a limited number of specimens can be tested. The transfer of results from *in vitro* tests to clinical situations is also challenging. FEA enables simulation of any situation, but the accuracy of the results depends on construction of an appropriate model. A meticulous construction process is therefore necessary. Previous works⁸⁻¹⁰ have combined the advantages of both methods to assess the effects of the material, and the dimensions, of the prefabricated posts. Teeth restored with stainless steel posts showed significantly lower failure loads than teeth restored with glass fibre posts. The experimental results were used to validate a finite element model of a restored tooth. From that model, it was concluded that post restoration systems, in which the elastic modulus of the post is similar to that of dentine and core, offer a better biomechanical performance. In these studies, a monotonic static load was applied, which does not represent the clinical situation (where a dynamic load is characteristic).

Fatigue tests have been established as being an essential research tool for testing adhesive restorations¹¹⁻¹⁹. They reproduce cyclical loading pattern comparable to physiological function and, therefore, can simulate the results of time-consuming clinical trials. More time could be saved if those tests were performed by means of computer simulation.

The purpose of this investigation was to compare the number of load cycles, without failure, sustained by a restored premolar (with a conventional complete crown design and two different post-and-core systems). The systems selected were: a prefabricated stainless steel

post and composite core, and a prefabricated glass fibre post and composite core.

MATERIALS AND METHODS

A theoretical method was used to study the influence of post material on endodontically treated, and restored with a post-core-crown system, human premolars. The posts used for the study were the *ParaPost Fiber White* and the *ParaPost Stainless Steel* (Coltène/Whaledent Inc, Mahwah, NJ, USA). These posts were selected because their geometry is similar and they are manufactured in the same sizes, but have significantly different elastic moduli (20 GPa for the *ParaPost Fiber White* and 207 GPa for the *Parapost Stainless Steel*).

Finite element model

The finite element analysis (FEA) is currently used in very different fields. It has been successfully used in biomechanics and, in particular, in orthopaedics. This technique was originally developed for structural analysis in mechanical engineering, but its foundation is also applicable to biological problems. The results of a FEA are expressed as stresses distributed in the structures under investigation. These stresses may be tensile, compressive, shear, or a combination known as equivalent von Mises stress. Von Mises stresses depend on the entire stress field and are a widely used indicator of the possibility of damage occurrence²⁰.

The model used in this study was based on the geometry of a real tooth, obtained through a 3D scanner, and the 3D modelling software Pro/Engineer (PTC, Needham, MA, USA) was used to generate, and later assemble, the geometries for all the components. This model has been properly validated in previous works⁸⁻¹⁰. Figure 1 shows a longitudinal section of the geometrical model considered, including all the components that were modelled: bone (cortical and trabecular components), periodontal ligament, root, gutta-percha, post, post cement, core, crown and crown cement. The mechanical

properties of the different components of the model were obtained from the literature and from the manufacturer of the posts (Coltène/Whaledent Inc, Mahwah, NJ, USA) and from the manufacturer of the glass-ceramic crown (Ivoclar Vivadent AG, Schaan, Liechtenstein). The aforementioned properties are presented in Table 1.

The Pro/Mechanica module, available within Pro/Engineer, was used to divide (mesh) the CAD geometry. Solid tetrahedral elements were created with a mesh control of 0.3 mm maximal size on all the components, except on trabecular and cortical bone, where a 1 mm maximal size control was applied. The definitive model had 216 173 elements. As boundary conditions, the displacements of all nodes on the lateral surface and base of the component representing the bone were constrained.

The analysis was carried out using the finite element analysis software MSC-PATRAN-NASTRAN (MSC).

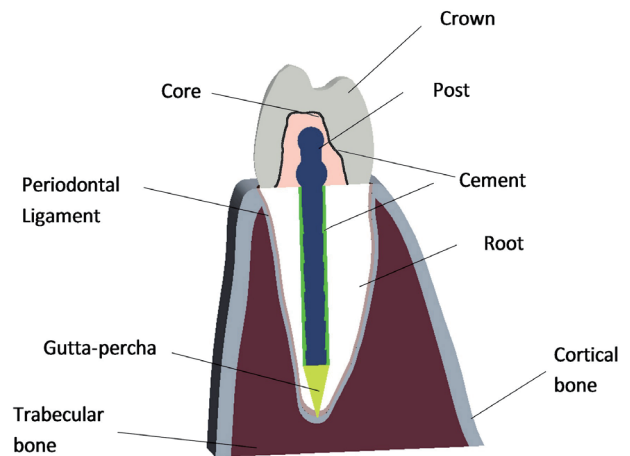


Fig. 1 Section of the geometrical model generated. Modelled components.

Table 1 Mechanical properties of the materials used in the finite element model

Component/Material	Elastic Modulus E (GPa)	Poisson Coefficient (ν)	References
Root/Dentine	18.6	0.31	20,40-44)
Gutta-percha	0.00069	0.45	20,40-44)
Periodontal ligament	0.0689	0.45	42,45)
Cortical bone	13.7	0.30	20,40-44)
Trabecular bone	1.37	0.30	20,40-44,46)
Post cement/Self cure resin cement	5	0.30	47)
Core/ParaPost ParaCore	20	0.30	Manufacturer
Crown	62	0.30	Manufacturer
Crown cement/Dual cement	10	0.30	47)
Stainless steel post	207	0.30	Manufacturer
Glass fibre post	20	0.30	Manufacturer

Software Corporation, Santa Ana, CA, USA). The study was undertaken with a model of a maxillary premolar restored using the *ParaPost Fiber White* and the *ParaPost Stainless Steel*, and with the definitive crown added. A 50 N load was applied to the palatal side of the tooth at a 30° angle to the radicular axis, in the vestibular direction, in order to simulate real biting force's direction²¹⁻²³. An unfavourable situation of malocclusion has been considered, *i.e.*, the force was applied to the buccal incline of the palatal cusp. The value of the occlusal force was chosen to represent a relatively high biting force²⁴. This value has been used in several works dealing with premolars^{16,25-27}. Under this load, the stress distribution pattern of the restored tooth was studied for two different post materials. The stress distribution pattern provided information about the fracture mechanism of the restored tooth: for the same external load, higher stresses indicated a higher probability of reaching the failure load.

As biomechanical performance was not found to depend on post length⁹, the widespread recommendation²⁸ that post length should be about three quarters of root length was used. The post diameter,

considered in this work, satisfies the widely extended recommendation that post width should not be greater than one-third of the root width at its narrowest section^{29,30}. Namely, the thickness ratio (post diameter/root thickness) chosen was equal to 0.2.

Fatigue Model from previous FEA

The behaviour of materials under dynamic loads is different to that under static loads. Fatigue can be defined as the progressive and localized structural damage that occurs when a material is subjected to cyclical loading³¹. The material collapses at maximum stress values that are lesser than the ultimate tensile stress limit, and may be below the yield stress limit of the material.

The von Mises stresses, obtained from the previous finite element analyses, were used through the COSMOSWorks module, available within the modelling software SolidWorks (Dassault Systèmes SolidWorks Corp., Suresnes, France). The S-N curves (Stress vs. Number of Cycles to Failure) were defined for each of the materials considered in the model. The S-N curve for dentine was obtained from the literature³². The S-N

Table 2 Flexural strengths for the different component materials of the model

	Flexural strength (MPa)	Source
ParaPost Fiber White	990	Manufacturer
ParaPost Stainless Steel	1,436	Manufacturer
ParaCore	90	48)
Dual Cement	45.1	47)
Dentine	212.9	49)
Crown	160	Manufacturer
Parapost Cement	97	50)

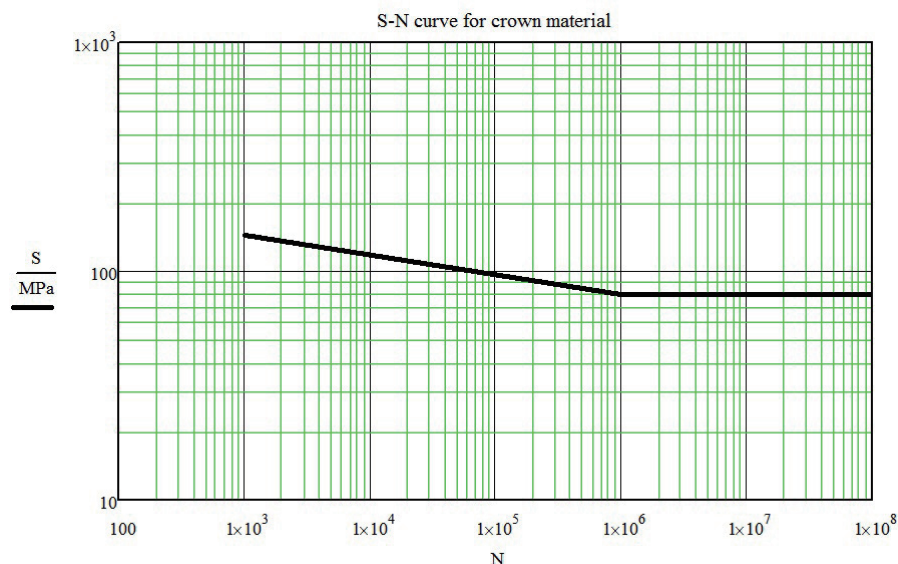


Fig. 2 S-N curve for crown material.

curves for the other materials were estimated from their static properties and S-N curves of similar materials found in the literature^{33,34}, *i.e.*, the S-N curve of materials, when no experimental data are available, is approximated by the following data (strength *versus* number of cycles): ($0.9 \cdot S_f$ vs. 10^3), ($0.5 \cdot S_f$ vs. 10^6) and ($0.5 \cdot S_f$ vs. a number of cycles greater than those tested). In this paper, we have tested 1.2 millions of cycles. S_f is the flexural strength of the material considered, shown in Table 2. As an example, Figure 2 shows the S-N curve for crown material.

A cyclical load, from 0 to 50 N, was applied during 1.2 millions of cycles. These conditions are believed to simulate, approximately, 5 years of clinical service³⁵. This number of cycles have been used in several fatigue studies^{12-16,36,37}. Taking into account that dental materials are brittle, the Goodman³¹ model was used for comparing the stresses obtained (in the previous finite element analyses) with the S-N curves.

RESULTS

Results from the static finite element analysis

In this section, the results of the study of the influence of the post material are presented. Figure 3 shows the stress distribution achieved. We prefer the more visual option of presenting the FOS (Factor of Safety) distribution. The FOS, for each component, has been calculated as the ratio between the strength of the component material and the maximal von Mises stress (obtained with the finite element model) in that component. Flexural strengths of each component material, obtained from literature, are presented in Table 2. A smaller factor of safety means that the component is more prone to failure. The smallest FOS of the components can be considered as the factor of safety of the overall system. As the saying goes, “A chain is only as strong as its weakest link”.

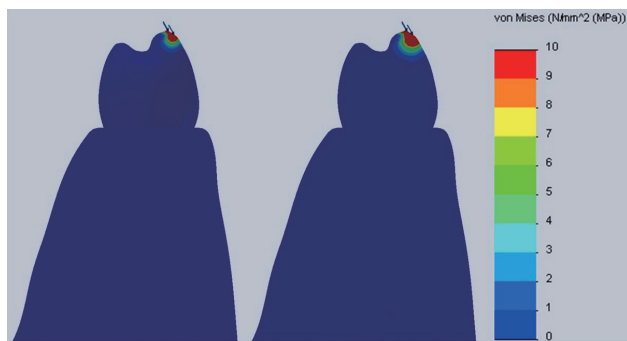


Fig. 3 von Mises stress distribution (colour scale: the warmer the colour, the higher the stress) estimated by the model for the restored tooth, on the sagittal section: using glass fibre post (left) vs. using stainless steel post (right).

For both post systems (Fig. 4), the smallest factors were located at the force application zone. Nonetheless, in the tooth restored with a stainless steel post, the extension of the zone with the smallest factors of safety is bigger. *i.e.*, the model predicts that restorations using glass fibre posts are able to bear higher static loads.

Results from the fatigue model from previous FEA

The model predicted no fatigue failure for both post systems studied, under the cyclical load considered (Fig. 5). That means that, although restorations using glass fibre posts are able to bear higher static loads, both post systems will safely bear this cyclical load. If the cyclical load considered is good enough to represent the real case, then both systems could be used in practice with the same guaranties.

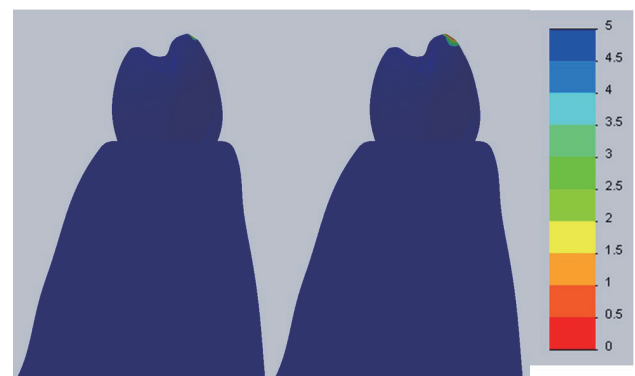


Fig. 4 Factor of safety (colour scale: the warmer the colour, the smaller the factor) estimated by the model for the restored tooth, on the sagittal section: using glass fibre post (left) and using stainless steel post (right).

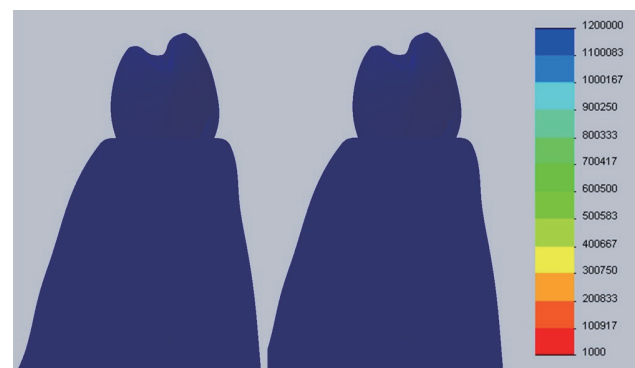


Fig. 5 Life prediction (*number of cycles*) for the cyclical load considered (colour scale: the warmer the colour, the shorter the life expected) estimated by the model for the restored tooth, on the sagittal section: using glass fibre post (left) vs. using stainless steel post (right).

DISCUSSION

In the present study, two different post systems models (glass fibre and stainless steel post) have been exposed to cyclic loading. Both post systems survived the cyclical load considered. That means that both systems would have a similar life, despite the differences found in the static analysis. It has to be pointed out that the results shown in this work have to be taken with care, because of the S-N curves that have been estimated.

The magnitude and direction of the force applied are comparable with values reported in the literature for premolars²¹⁻²³). The analysis of the factor of safety (under a static load) revealed that the failure would occur at the crown, in the area where the load is applied. In any case, the mode of failure predicted by the model for crowned restored teeth would not affect the root.

Many studies in the literature address fatigue of a core, supported by a post, experimentally¹¹⁻¹⁶). Nonetheless, most of them do not take into account the protective effect of the definitive crown in the restoration. In this way, their results are similar to that of the static studies, *i.e.*, post restoration systems, in which the elastic modulus of the post is similar to that of dentine and core, offer a better biomechanical performance^{8-10,38}). The work of Goto *et al.*³⁹) obtained that fibre-reinforced resin dowels and bonded composite cores, under fatigue loading, provided significantly stronger crown retention than cast gold dowels and cores and titanium alloy dowels with composite cores under fatigue loading. But retention is not an issue addressed in this work; we have dealt with the resistance of the post system.

Besides the usual limitations of finite element studies, one limitation of this work was the exclusive use of reinforced glass-ceramic crowns, for the definitive restoration of the root-canal-treated teeth. This only gives information about the tested combinations of posts, cores, and crowns, and the results cannot be generalized for other combinations, especially for other crowns made of metal, ceramic fused to metal or composite resin.

Although the method used is more clinically relevant than study methods employing a monotonic static load, limitations exist in the interpretation of these results from a clinical perspective. The specimens in this model were not subjected to thermal cycling, and the fatigue load was always applied in a uniform manner. Also, dentine bonding was accomplished under ideal conditions that may not fully represent the clinical situation.

The method proposed in this work, for studying the biomechanics of teeth restored using intraradicular posts, is easy to perform from a previous FEA. In addition, provide results more intuitive and easier to interpret. The results are more realistic because the method takes into account the dynamic nature of masticatory loads. The main limitation of the method is that requires S-N experimental curves of dental-restorative materials, which are not usually provided by manufacturers.

CONCLUSION

Both post systems considered (glass fibre and stainless steel post) would have a similar life, despite the differences found in the static analysis.

ACKNOWLEDGMENTS

This research is supported by both the Spanish Government and the European Union (FEDER funds) through Project DPI2006-13432.

REFERENCES

- 1) Gutman JL. The dentin-root complex: anatomic and biologic considerations in restoring endodontically treated teeth. *J Prosthet Dent* 1992; 67: 458-467.
- 2) Christensen GJ. Posts and cores: state of the art. *J Am Dent Assoc* 1998; 129: 96-97.
- 3) Robbins JW. Guidelines for the restoration of endodontically treated teeth. *J Am Dent Assoc* 1990; 120: 558, 560, 562 *passim*.
- 4) Sjogren G, Sletten G, Dahl JE. Cytotoxicity of dental alloys, metals, and ceramics assessed by Millipore filter, agar overlay, and MTT tests. *J Prosthet Dent* 2000; 84: 229-236.
- 5) Ku CW, Park SW, Yang HS. Comparison of the fracture strengths of metal-ceramic crowns and three ceromer crowns. *J Prosthet Dent* 2002; 88: 170-175.
- 6) Hwang JW, Yang JH. Fracture strength of copy-milled and conventional In-Ceram crowns. *J Oral Rehabil* 2001; 28: 678-683.
- 7) Fradeani M, Redemagni M. An 11-year clinical evaluation of leucite-reinforced glass-ceramic crowns: a retrospective study. *Quintessence Int* 2002; 33: 503-510.
- 8) Barjau-Escribano A, Sancho-Bru JL, Forner-Navarro L, Rodríguez-Cervantes PJ, Pérez-González A, Sánchez-Marín FT. Influence of prefabricated post material on restored teeth: fracture strength and stress distribution. *Oper Dent* 2006; 31: 47-54.
- 9) Rodríguez-Cervantes PJ, Sancho-Bru JL, Barjau-Escribano A, Forner-Navarro L, Pérez-González A, Sánchez-Marín FT. Influence of prefabricated post dimensions on restored maxillary central incisors. *J Oral Rehabil* 2007; 34: 141-152.
- 10) Gonzalez-Lluch C, Rodríguez-Cervantes PJ, Sancho-Bru JL, Perez-Gonzalez A, Barjau-Escribano A, Vergara-Monedero M, *et al.* Influence of material and diameter of pre-fabricated posts on maxillary central incisors restored with crown. *J Oral Rehabil* 2009; 36: 737-747.
- 11) Cohen BI, Pagnillo MK, Newman I, Musikant BL, Deutsch AS. Pilot study of the cyclic fatigue characteristics of five endodontic posts with four core materials. *J Oral Rehabil* 2000; 27: 83-92.
- 12) Buttel L, Krastl G, Lorch H, Naumann M, Zitzmann NU, Weiger R. Influence of post fit and post length on fracture resistance. *Int Endod J* 2009; 42: 47-53.
- 13) Okutan M, Heydecke G, Butz F, Strub JR. Fracture load and marginal fit of shrinkage-free ZrSiO₄ all-ceramic crowns after chewing simulation. *J Oral Rehabil* 2006; 33: 827-832.
- 14) Strub JR, Pontius O, Koutayas S. Survival rate and fracture strength of incisors restored with different post and core systems after exposure in the artificial mouth. *J Oral Rehabil* 2001; 28: 120-124.
- 15) Kern M, Strub JR, Lu XY. Wear of composite resin veneering materials in a dual-axis chewing simulator. *J Oral Rehabil* 1999; 26: 372-378.
- 16) Stricker EJ, Gohring TN. Influence of different posts and cores on marginal adaptation, fracture resistance, and

- fracture mode of composite resin crowns on human mandibular premolars. An *in vitro* study. J Dent 2006; 34: 326-335.
- 17) Guess P, Zavanelli R, Silva N, Bonfante E, Coelho P, Thompson V. Monolithic CAD/CAM lithium disilicate *versus* veneered Y-TZP crowns: Comparison of failure modes and reliability after fatigue. Int J Prosthodont 2010; 23: 434-442.
 - 18) Chaibabutr Y, Phillips K, Ma P, ChitSwe K. Comparison of load-fatigue testing of ceramic veneers with two different preparation designs. Int J Prosthodont 2009; 22: 573-575.
 - 19) Baldissara P, Di Grazia V, Palano A, Ciocca L. Fatigue resistance of restored endodontically treated teeth: a multiparametric analysis. Int J Prosthodont 2006; 19: 25-27.
 - 20) Pegoretti A, Fambri L, Zappini G, Bianchetti M. Finite element analysis of a glass fibre reinforced composite endodontic post. Biomaterials 2002; 23: 2667-2682.
 - 21) Assif D, Oren E, Marshak BL, Aviv I. Photoelastic analysis of stress transfer by endodontically treated teeth to the supporting structure using different restorative techniques. J Prosthet Dent 1989; 61: 535-543.
 - 22) Cohen BI, Pagnillo MK, Newman I, Musikant BL, Deutsch AS. Cyclic fatigue testing of five endodontic post designs supported by four core materials. J Prosthet Dent 1997; 78: 458-464.
 - 23) Fokkinga WA, Le Bell AM, Kreulen CM, Lassila LV, Vallittu PK, Creugers NH. Ex vivo fracture resistance of direct resin composite complete crowns with and without posts on maxillary premolars. Int Endod J 2005; 38: 230-237.
 - 24) Hattori Y, Satoh C, Kunieda T, Endoh R, Hisamatsu H, Watanabe M. Bite forces and their resultants during forceful intercuspal clenching in humans. J Biomech 2009; 42: 1533-1538.
 - 25) Rundquist BD, Versluis A. How does canal taper affect root stresses? Int Endod J 2006; 39: 226-237.
 - 26) Jensen AL, Abbott PV. Experimental model: dye penetration of extensive interim restorations used during endodontic treatment while under load in a multiple axis chewing simulator. J Endod 2007; 33: 1243-1246.
 - 27) Schmitter M, Rammelsberg P, Lenz J, Scheuber S, Schweizerhof K, Rues S. Teeth restored using fiber-reinforced posts: *In vitro* fracture tests and finite element analysis. Acta Biomater 2010; 6: 3747-3754.
 - 28) Smith CT, Schuman NJ, Wasson W. Biomechanical criteria for evaluating prefabricated post-and-core systems: a guide for the restorative dentist. Quintessence Int 1998; 29: 305-312.
 - 29) Nergiz I, Schmager P, Ozcan M, Platzter U. Effect of length and diameter of tapered posts on the retention. J Oral Rehabil 2002; 29: 28-34.
 - 30) Stern N, Hirshfeld Z. Principles of preparing endodontically treated teeth for dowel and core restorations. J Prosthet Dent 1973; 30: 162-165.
 - 31) Lee U: Fatigue testing and analysis: theory and practice, Burlington, Elsevier Butterworth-Heinemann, 2005, p. 1-402.
 - 32) Arola D, Replogel RK. Effects of aging on the mechanical behavior of human dentin. Biomaterials 2005; 26: 4051-4061.
 - 33) Baran G, Boberick K, McCool J. Fatigue of restorative materials. Crit Rev Oral Biol Med 2001; 12: 350-360.
 - 34) Grandini S, Chieffi N, Cagidiaco MC, Goracci C, Ferrari M. Fatigue resistance and structural integrity of different types of fiber posts. Dent Mater J 2008; 27: 687-694.
 - 35) Krejci I, Mueller E, Lutz F. Effects of thermocycling and occlusal force on adhesive composite crowns. J Dent Res 1994; 73: 1228-1232.
 - 36) Heydecke G, Butz F, Hussein A, Strub JR. Fracture strength after dynamic loading of endodontically treated teeth restored with different post-and-core systems. J Prosthet Dent 2002; 87: 438-445.
 - 37) Nothdurft FP, Schmitt T, Rupf S, Pospiech PR. Influence of fatigue testing and cementation mode on the load-bearing capability of bovine incisors restored with crowns and FRC posts. Dent Mater J 2011; 30: 109-114.
 - 38) Rodríguez-Cervantes PJ, González-Lluch C, Sancho-Bru JL, Barjau-Escribano A, Pérez-González A, Forner-Navarro L: Biodental Engineering, Boca Raton, FL, USA, CRC Press-Taylor & Francis Group, 2010, p. 41-46.
 - 39) Goto Y, Nicholls JJ, Phillips KM, Junge T. Fatigue resistance of endodontically treated teeth restored with three dowel-and-core systems. J Prosthet Dent 2005; 93: 45-50.
 - 40) Dejak B, Mlotkowski A, Romanowicz M. Finite element analysis of stresses in molars during clenching and mastication. J Prosthet Dent 2003; 90: 591-597.
 - 41) Dejak B, Mlotkowski A, Romanowicz M. Finite element analysis of mechanism of cervical lesion formation in simulated molars during mastication and parafunction. J Prosthet Dent 2005; 94: 520-529.
 - 42) Boschian Pest L, Guidotti S, Pietrabissa R, Gagliani M. Stress distribution in a post-restored tooth using the three-dimensional finite element method. J Oral Rehabil 2006; 33: 690-697.
 - 43) Holmes DC, Diaz-Arnold AM, Leary JM. Influence of post dimension on stress distribution in dentin. J Prosthet Dent 1996; 75: 140-147.
 - 44) Asmussen E, Peutzfeldt A, Heitmann T. Stiffness, elastic limit, and strength of newer types of endodontic posts. J Dent 1999; 27: 275-278.
 - 45) Asmussen E, Peutzfeldt A, Sahafi A. Finite element analysis of stresses in endodontically treated, dowel-restored teeth. J Prosthet Dent 2005; 94: 321-329.
 - 46) Eskitascioglu G, Usumez A, Sevimay M, Soykan E, Unsal E. The influence of occlusal loading location on stresses transferred to implant-supported prostheses and supporting bone: A three-dimensional finite element study. J Prosthet Dent 2004; 91: 144-150.
 - 47) Saskalauskaitė E, Tam LE, McComb D. Flexural strength, elastic modulus, and pH profile of self-etch resin luting cements. J Prosthodont 2008; 17: 262-268.
 - 48) Dodiuk-Kenig H, Lizenboim K, Eppelbaum I, Zalsman B, Kenig S. The effect of hyper-branched polymers on the properties of dental composites and adhesives. J Adhes Sci Tech 2004; 18: 1723-1737.
 - 49) Plotino G, Grande NM, Bedini R, Pameijer CH, Somma F. Flexural properties of endodontic posts and human root dentin. Dent Mater 2007; 23: 1129-1135.
 - 50) Baudin II G, Burgess JO. Flexural strength of fourteen cements. J Dent Res 2002; 81: 169.